



**HD 2108.1, HD 2108.2, HD 2128.1, HD2128.2  
THERMOCOUPLE THERMOMETERS: K, J, T, N, R, S, B, E**

The HD2108.1 and HD2108.2 **with one input** and the HD2128.1 and HD2128.2 **with two inputs** are portable instruments with a large LCD display. They measure the temperature using immersion, penetration, air or contact probes. The sensor may be a thermocouple of type K, J, T, N, R, S, B or E.

Instruments HD2108.2 and HD2128.2 are **data logger**, they store up to 76.000 samples the first and 38.000 couples of values the second. These data can be transferred into a PC connected to the instrument through the serial ports RS232C and USB 2.0. It is possible to configure the storage interval, the printing and the baud rate by the menu.

All models are equipped with RS232C serial port and are able to transfer the acquired measures, in real time, to a PC or a portable printer.

Functions Max, Min and Avg calculate maximum, minimum and average values. Further functions are: REL relative measure, HOLD and automatic switching-off system, excludable. HD2128.1 and HD2128.2 calculate A-B difference of the temperatures acquired by the two input channels.

**Instruments have IP66 protection degree.**



HD2108



HD2128

	HD2108.1	HD2108.2	HD2128.1	HD2128.2
<b>TC input:</b>	1	1	2	2
<b>Storage capacity</b>	----	76000 samples	----	38000 couples of temperatures
<b>PC interface</b>	RS232C	RS232C + USB2.0	RS232C	RS232C + USB2.0
<b>Data logger</b>	NO	YES	NO	YES
<b>A-B function</b>	NO	NO	YES	YES

**TECHNICAL SPECIFICATIONS OF THE INSTRUMENTS**

*Instrument*

**Dimensions**  
(Length x Width x Height) 185x90x40mm  
**Weight** 470g (complete with Batteries)  
**Materials** ABS, rubber  
**Display** 2x4½ digits plus symbols  
Visible area: 52x42mm

*Operating conditions*

**Operating temperature** -5 ... 50°C  
**Storage temperature** -25 ... 65°C  
**Working relative humidity** 0 ... 90% RH, no condensation  
**Protection degree** **IP66**

*Power supply*

**Batteries** 4 Batteries 1.5V type AA  
**Autonomy** 200 hours with 1800mAh alkaline batteries  
**Current consumption with instrument off** 20µA  
**Main** 12Vdc / 1000mA Output main adapter

*Unit of measurement*

°C - °F - °K - mV - mV°C

*Security of stored data*

Unlimited, independent of battery charge conditions  
1min/month max drift

*Time*

**Date and time** In real time  
**Accuracy** 1min/month max drift

*Measured values storage*

**Model HD2108.2** 2000 pages each one containing 38 samples, 76000 samples in total

**Model HD2128.2** 2000 pages each one containing 19 samples, 38000 couples of samples

**Storage interval can be selected between** 1,5,10,15,30 s.; 1,2,5,10,15,20,30 min.; 1 hour

*Serial interface RS232C*

**Type** RS232C galvanically isolated  
**Baud rate** can be set from 1200 to 38400 baud  
**Data bit** 8  
**Parity** None  
**Stop bit** 1  
**Flow Control** Xon/Xoff  
**Serial cable length** Max 15m  
**Print interval** Immediate selectable between 1,5,10,15,30 s.; 1,2,5,10,15,20,30 min.; 1 hour

*USB interface - model HD2108.2 and HD2128.2*

**Type** 1.1 - 2.0 galvanically isolated

*Connections*

**Probes input** 2-pole female polarized standard miniature connector  
**Serial interface** 8-pole MiniDin connector  
**USB interface** Type B Mini USB connector  
**Mains adapter** 2-pole connector (positive at centre)

### Measurement of temperature by Instrument

TC measuring range: K	-200...+1370°C
TC measuring range: J	-100...+750°C
TC measuring range: T	-200...+400°C
TC measuring range: N	-200...+1300°C
TC measuring range: R	+200...+1480°C
TC measuring range: S	+200...+1480°C
TC measuring range: B	+200...+1800°C
TC measuring range: E	-200...+750°C

### Resolution

**0.05°C up to 199.95°C**  
**0.1°C from 200.0°C up to full scale**

### Instrument accuracy

Thermocouple K	±0.1°C up to 600°C ±0.2°C over 600°C
Thermocouple J	±0.05°C up to 400°C ±0.1°C over 400°C
Thermocouple T	±0.1°C
Thermocouple N	±0.1°C up to 600°C ±0.2°C over 600°C
Thermocouple R	±0.25°C
Thermocouple S	±0.3°C
Thermocouple B	±0.35°C
Thermocouple E	±0.1°C up to 300°C ±0.15°C over 300°C

**Accuracy is referred to the instrument only; error due to the thermocouple or to the cold junction reference sensor is not included.**

Temperature drift @20°C	0.02%/°C
Drift after 1 year	0.1°C/year

### Thermocouple probes accuracy:

Tolerance of a type of thermocouple corresponds to the maximum acceptable shift from the e.m.f. of any thermocouple of that type, with reference junction at 0°C. The tolerance is expressed in degrees Celsius, preceded by the sign. The percentage tolerance is given by the ratio between the tolerance expressed in degrees Celsius and the measurement junction temperature, multiplied by one hundred.

The tolerances refer to the operating temperature expected for the thermocouple, in agreement with the thermo-elements' diameter.

Those thermocouples that comply with the limits for temperatures over 0°C, do not necessarily comply with the limits for ranges below 0°C.

### Tolerance classes for thermocouples (reference junction at 0°C)

Type of thermocouple	Tolerance Class 1	Tolerance Class 2	Tolerance Class 3 <sup>(1)</sup>
<b>Type T</b> Temperature interval Tolerance Temperature interval Tolerance	from -40 to +125°C ± 0.5°C from 125 to 350°C ± 0.004 · t	from -40 to +133°C ± 1°C from 133 to 350°C ± 0.0075 · t	from -67 to +40°C ± 1°C from -200 to -67°C ± 0.015 · t
<b>Type E</b> Temperature interval Tolerance Temperature interval Tolerance	from -40 to +375°C ± 1.5°C from 375 to 800°C ± 0.004 · t	from -40 to +333°C ± 2.5°C from 333 to 900°C ± 0.0075 · t	from -167 to +40°C ± 2.5°C from -200 to -167°C ± 0.015 · t
<b>Type J</b> Temperature interval Tolerance Temperature interval Tolerance	from -40 to +375°C ± 1.5°C from 375 to 750°C ± 0.004 · t	from -40 to +333°C ± 2.5°C from 333 to 750°C ± 0.0075 · t	- - - -
<b>Type K, type N</b> Temperature interval Tolerance Temperature interval Tolerance	from -40 to +375°C ± 1.5°C from 375 to 1000°C ± 0.004 · t	from 40 to +333°C ± 2.5°C from 333 to 1200°C ± 0.0075 · t	from -167 to +40°C ± 2.5°C from -200 to -167°C ± 0.015 · t
<b>Type R, type S</b> Temperature interval Tolerance Temperature interval Tolerance	from 0 to +1100°C ± 1°C from 1100 to 1600°C ± [ 1 + 0.003 (t-1100)] °C	from 0 to +600°C ± 1.5°C from 600 to 1600°C ± 0.0025 · t	- - - -
<b>Type B</b> Temperature interval Tolerance Temperature interval Tolerance	- - - -	- - from 600 to 1700 °C ± 0.0025 · t	from +600 to +800C + 4°C from 800 to 1700°C ± 0.005 · t

<sup>(1)</sup> Materials for thermocouples are generally supplied so to comply with the factory tolerances specified in the table for temperatures over -40°C. However these materials can sometimes not comply with the factory tolerances for the low temperatures reported under Class 3, for thermocouples of T, E, K and N type, when thermocouples have to comply at the same time the limits of Class 3 and Class 1 and/or Class 2.



CP23



HD40.1

## ORDERING CODES

**HD2108.1:** The kit consists of **one input** instrument HD2108.1, 4 per 1.5V alkaline batteries, instruction manual, case and DeltaLog9 software. **Probes and cables have to be ordered separately.**

**HD2108.2:** The kit consists of **one input** instrument HD2108.2, **data logger**, 4 per 1.5V alkaline batteries, instruction manual, case and DeltaLog9 software. **Probes and cables have to be ordered separately.**

**HD2128.1:** The kit consists of **two inputs** instrument HD2128.1, 4 per 1.5V alkaline batteries, instruction manual, case and DeltaLog9 software. **Probes and cables have to be ordered separately.**

**HD2128.2:** The kit consists of **two inputs** instrument HD2128.2, **data logger**, 4 per 1.5V alkaline batteries, instruction manual, case and DeltaLog9 software. **Probes and cables have to be ordered separately.**

**HD2110CSNM:** 8-pole connection cable MiniDin - Sub D 9-pole female for RS232C.

**C.206:** Cable for instruments of the serie HD21...1 to connect directly to USB input of PC.

**CP23:** Connection cable USB 2.0 connector type A - Mini USB type B.

**DeltaLog9:** Software for download and management of the data on PC using Windows® operating systems.


**SWD10:** Stabilized power supply at 230Vac/12Vdc-1000mA mains voltage.

**HD40.1:** Upon request, portable, thermal printer, 24 column thermal printer, 58mm paper width. Use cable HD2110CSNM (option).

## Thermocouple probes

**Any thermocouple probe with standard miniature connector available on the price list can be connected to these instruments.**

**Please see pages from TP- 15 to TP-19.**

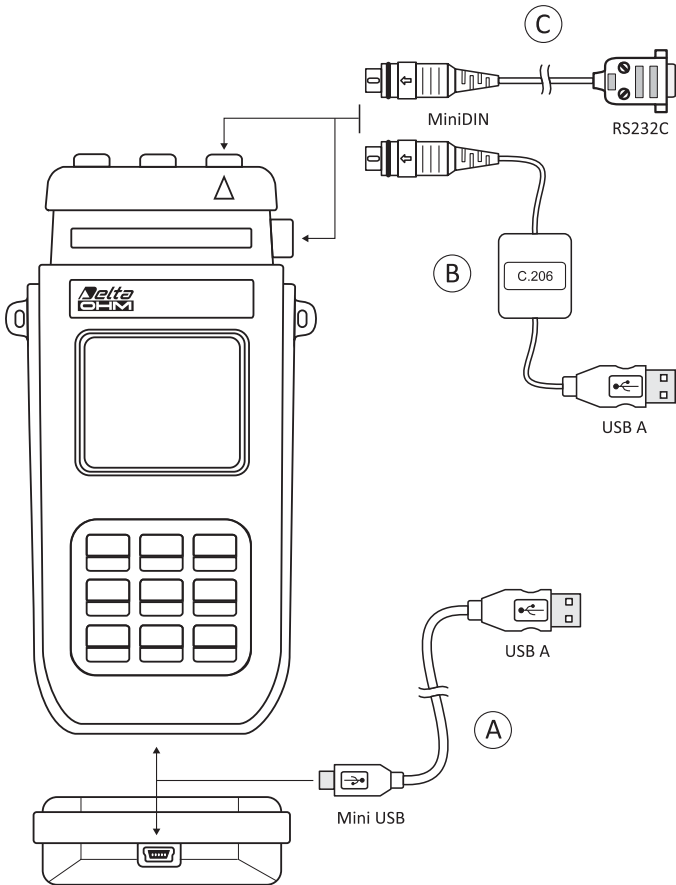

**A** To the portable data loggers of the series **HD21...2** a serial port mini USB type HID (Human Interface Device) has been inserted.

For the connection to a PC with the cable USB type A - MiniUSB type B code CP23, **it is not necessary to load any driver USB.**

**B** For the connection of the models **HD21...1** to the USB port of a PC, is necessary the USB/serial converter **C.206**. The converter is supplied with its own drivers which must be installed before the connection of the converter to the PC.(see details in the Cd-Rom supplied with the converter).

**C** The port with the miniDin connector in all the models, is a serial port type RS232C. The serial port RS232C of a PC or the printer HD40.1 can be connected by the cable HD2110CSNM.



SWD10



HD2110CSNM